



INDOFINE Chemical Company, Inc.

121 Stryker Lane Hillsborough, NJ 08844 USA

Phone: (908) 359-6778; Fax: (908) 359-1179


ANALYTICAL CONDITIONS

GC ANALYSIS

α -(-)-BISABOLOL

025244S Batch: 21

COLUMN Capillary 60m DB-WAX
TEMPERATURE Column : 50 to 220°C (6°C/min)
DETECTOR FID
CARRIER GAS N₂ 1.0 bar

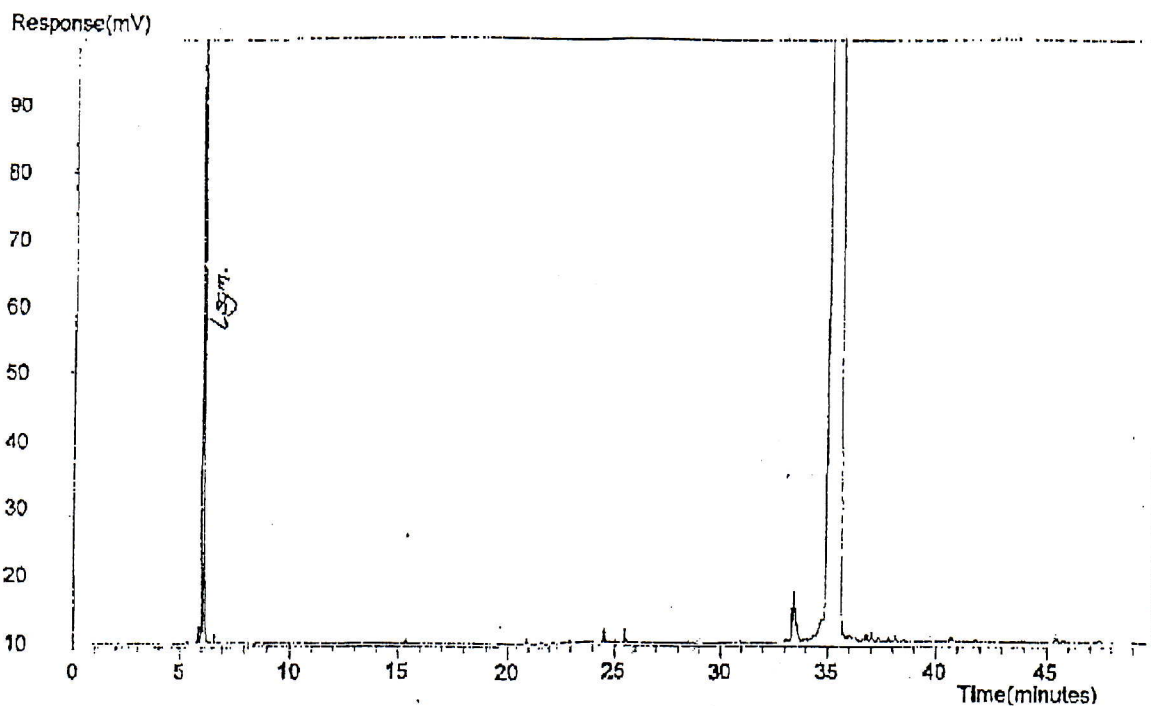

RT	AREA	% AREA
33,38	23,26	0,32
33,49	59,45	0,81
34,76	54,28	0,74
35,63	7218,66	98,14