



INDOFINE Chemical Company, Inc.

121 Stryker Lane, Bldg. 30
Hillsborough, NJ 08844 USA
Phone: (908) 359-6778; Fax: (908) 359-1179

ANALYTICAL CONDITIONS

G C ANALYSIS

alpha(-)-BISABOLOL

025244S Batch: 22


COLUMN Carbowax Capillary
 30 m x 0.32 mm x 0.25 µm

TEMPERATURE Column : 70 to 220°C (5°C/min)
 Injector:200°C
 Detector :230°C

DETECTOR FID

CARRIER GAS Hydrogen 6psi

SAMPLE SOLVENT Isopropanol

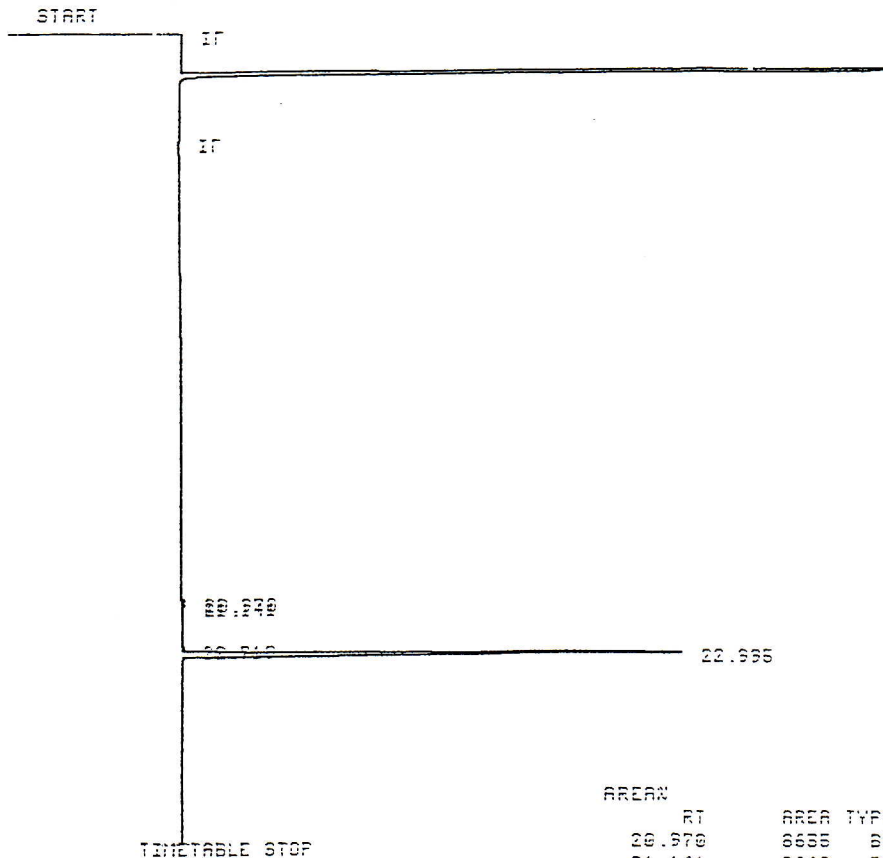

RT	AREA	TYPE	WIDTH	AREA%
20.970	6656	BP	.055	.42366
21.141	6649	FB	.057	.42438
22.719	14545	FU	.107	.70366
22.995	2006407	UB	.105	96.44836