INDOFINE Chemical Company, Inc.

121 Stryker Lane, Bldg. 30, Suite 1 • Hillsborough, NJ 08844 • U.S.A.
Phone: (908) 359-6778 • FAX: (908) 359-1179
website: www.indofinechemical.com
e-mail: chemical@indofinechemical.com

14-0803 3-Hydroxyoctanoic Acid
GC Methylated sample

Lot no: J 273:9
Purity: 98+ %
Storage: Freezer

GC:
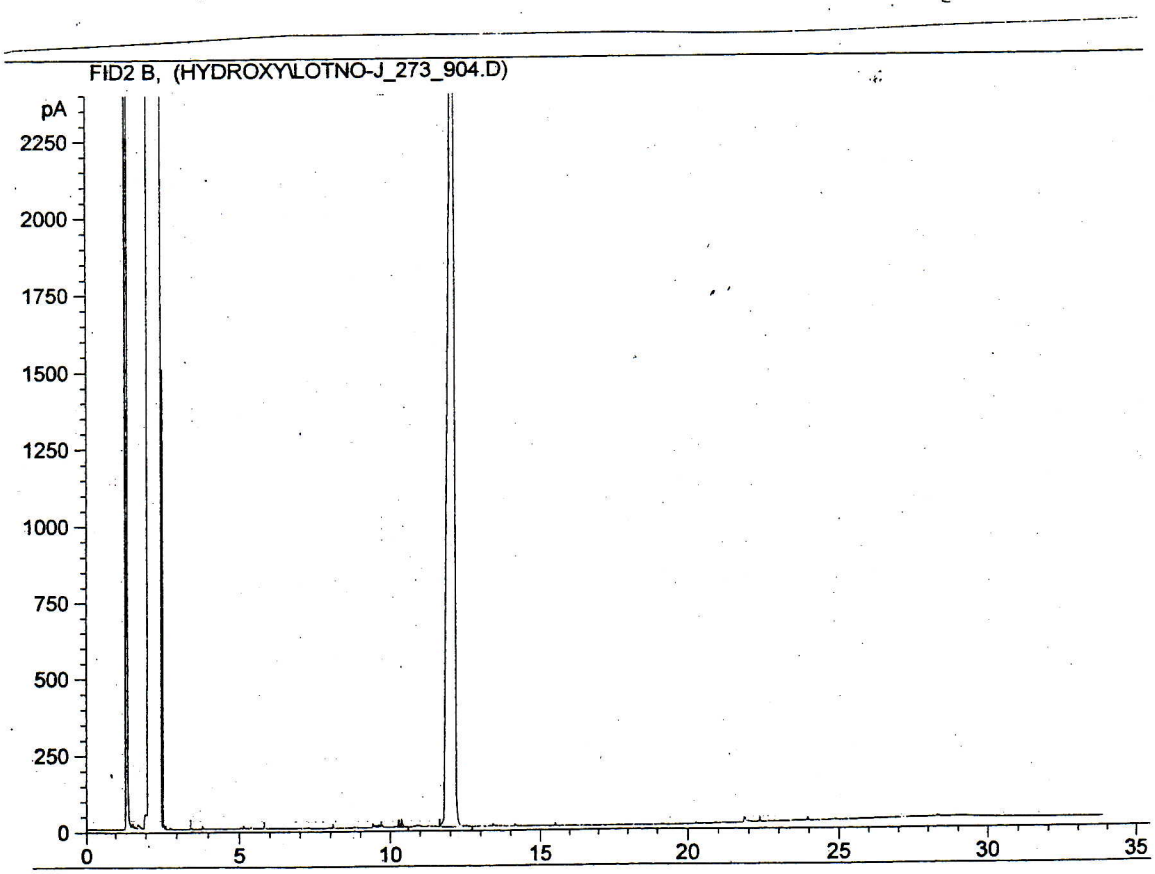
Injection	:	On column
Detector	:	FID
Column	:	HP-5 30m x 0.32mm film 0.25um
Carrier	:	Helium 14psi
Temperature		
Column		
Initial	:	50°C 3 min
Final	:	260°C
Rate	:	10°C/min.
Injector	:	240°C
Detector	:	270°C